

---

.....	1
.....	2
.....	3
.....	4

, BioStar 2,

(Alert History) 가 BioStar 2 BioStar 2


Date	Device	User	Alarm	Ack. By	Status
2016/08/02 11:40:14	BioStation A2 541531090 (192...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/08/02 11:40
2016/08/02 11:44:33	BioStation A2 541531090 (192...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/08/02 11:45
2016/08/01 10:28:14	BioStation A2 541531090 (192... 838974592(-)		1:1 authentication failed (Card)	Administrator (High...	2016/08/01 10:30
2016/08/01 12:40:28	BioStation A2 541531090 (192... 468846592(-)		1:1 authentication failed (Card)	Administrator (High...	2016/08/01 12:49
2016/08/01 10:42:41	BioStation A2 541531090 (192... 88889840(-)		1:1 authentication failed (Card)	Administrator (High...	2016/08/01 11:17
2016/08/01 09:35:42	BioStation A2 541531090 (192...		Device restarted	Administrator (High...	2016/08/01 09:39
2016/08/01 09:30:18	BioStation A2 541531090 (192...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/08/01 09:30
2016/08/01 09:29:48	BioStation A2 541531090 (192...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/08/01 09:29
2016/07/29 16:40:17	BioStation 2 548832593 (192.1...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/07/29 16:40
2016/07/29 16:40:27	BioStation 2 548832593 (192.1...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/07/29 16:40
2016/07/29 16:39:59	BioStation 2 548832593 (192.1...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/07/29 16:40
2016/07/29 16:39:41	BioStation 2 548832593 (192.1...		1:N authentication failed (Fingerprint)	Administrator (High...	2016/07/29 16:39
2016/07/29 15:48:48	BioStation 2 548832593 (192.1... 123864318(-)		1:1 authentication failed (Card)	Administrator (High...	2016/07/29 15:48
2016/07/29 15:22:51	BioJHelix 10200 (192.168.16... 187349648(-)		1:1 authentication failed (Card)	Administrator (High...	2016/07/29 15:22
2016/07/29 15:04:52	BioStation A2 541531090 (192...		Device restarted	AdminUser	2016/07/29 15:04
2016/07/29 15:00:53	BioStation 2 548832593 (192.1... 133967932(-)		1:1 authentication failed (Card)	Administrator (High...	2016/07/29 15:00
2016/07/29 14:05:14	BioStation 2 548832593 (192.1... 125864318(-)		1:1 authentication failed (Card)	Administrator (High...	2016/07/29 14:05
2016/07/29 14:05:59	BioStation 2 548832593 (192.168... 58752676(-)		1:1 authentication failed (Card)	Administrator (High...	2016/07/29 14:05

가 가

1. (Real-time Log) ( 가 )

Date	Door	Device ID	Device	User	Zone	Event	View
2016/08/02 11:44:33		541531090	BioStation A2 ...			1:N authentication failed (Fingerprint)	


2. (Ignore) ( 가 )가 (Acknowledge)

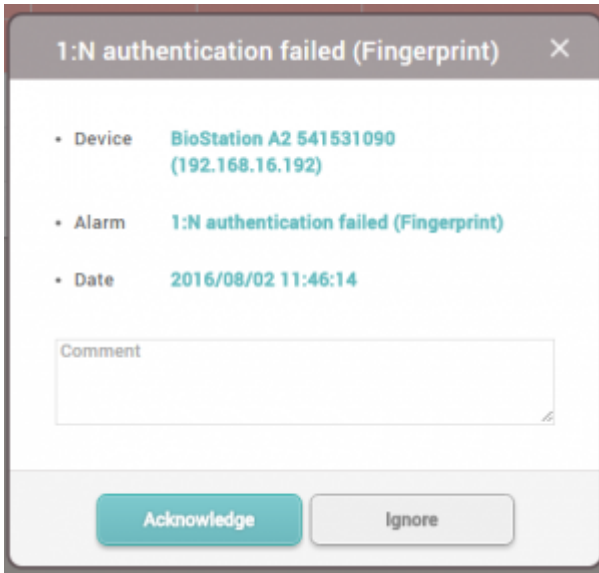


3. 가 가 .

BioStar 2 2.3


1. (Setting) > (ALERT)

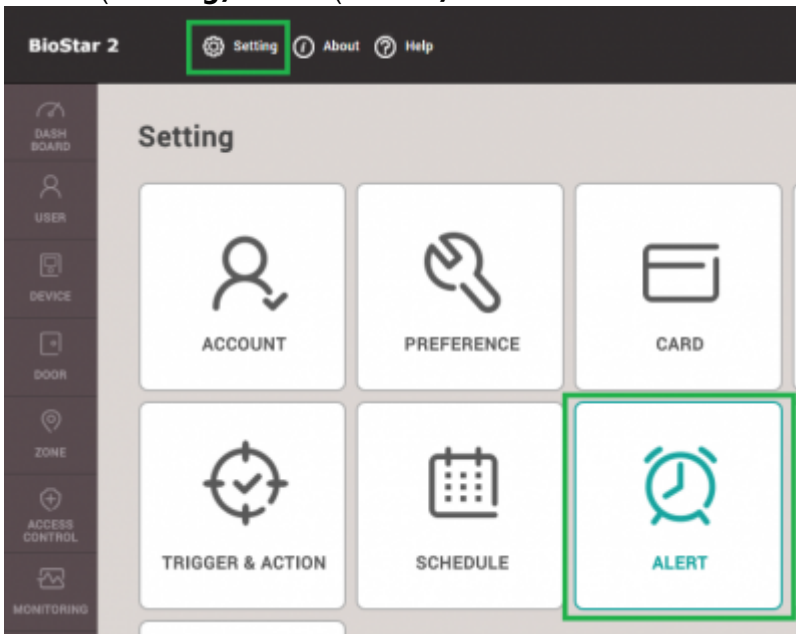


2. (Apply)

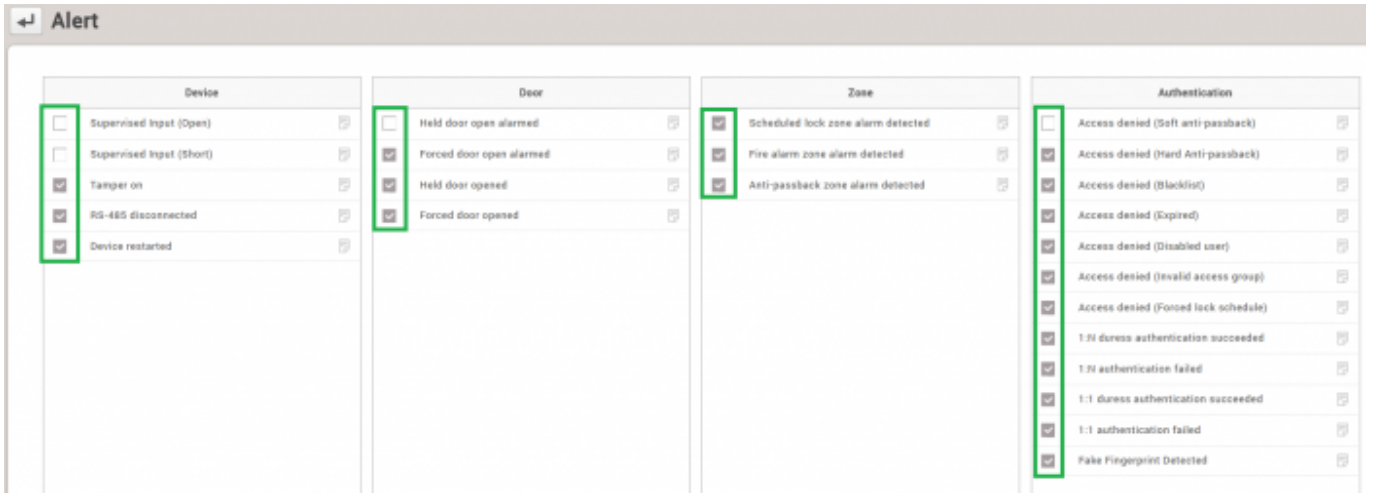


3. 가 (Real-time Log) 가

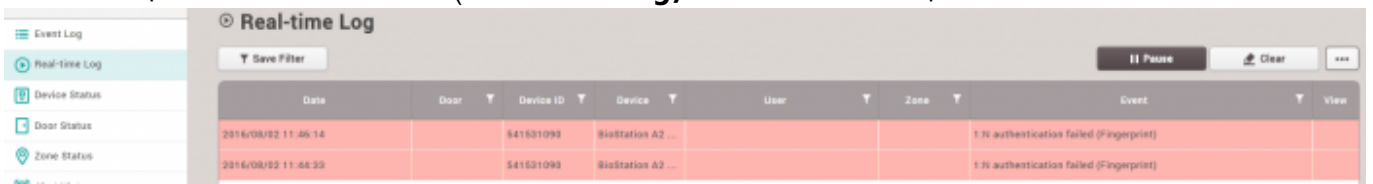


1. (Setting) > (ALERT)
- 2.




3. (Apply)

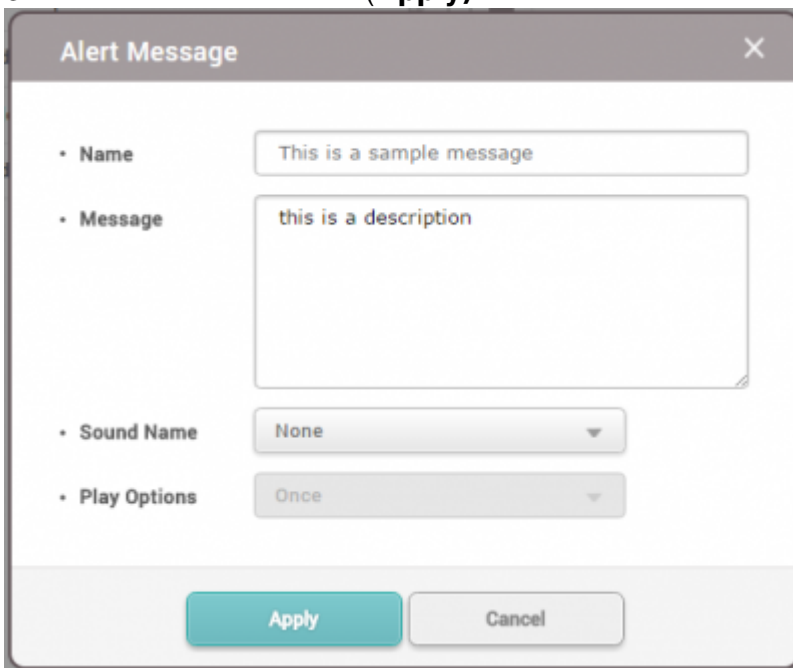

- 1. (Setting) > (PREFERENCE)
- 2. (Sound) + 가(+ Add)

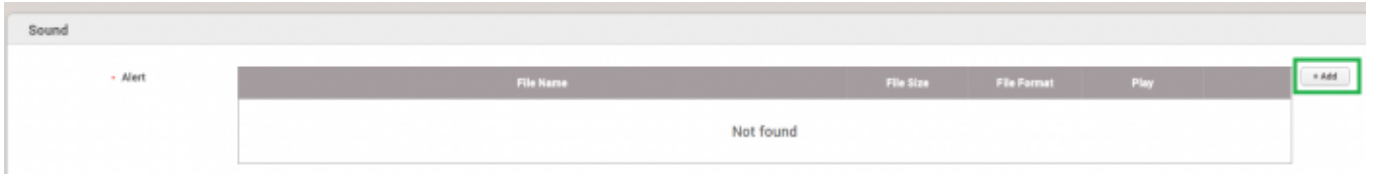


- 3. PC 가

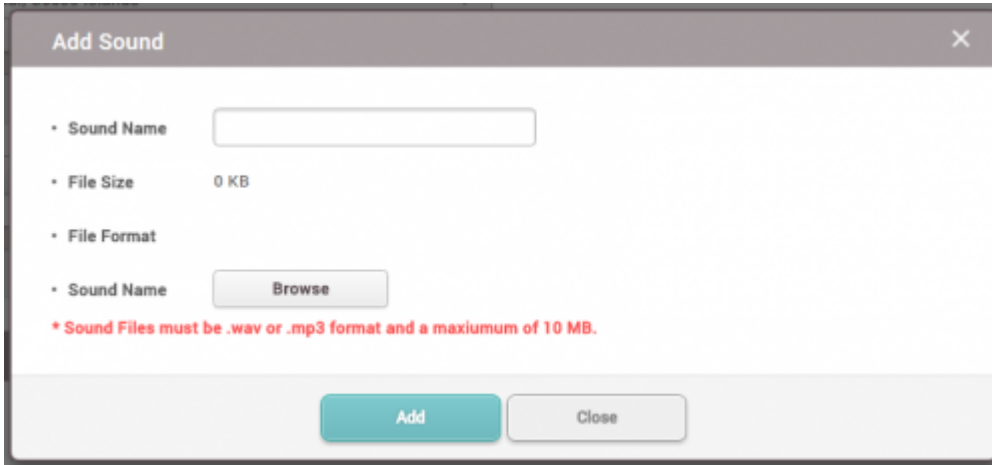

- 4. 가(Add) (Apply)
- 5. >
- 6.
- 7. (PREFERENCE) 가
- 8.

(Once) (Loop until acknowledge) (Acknowledge)

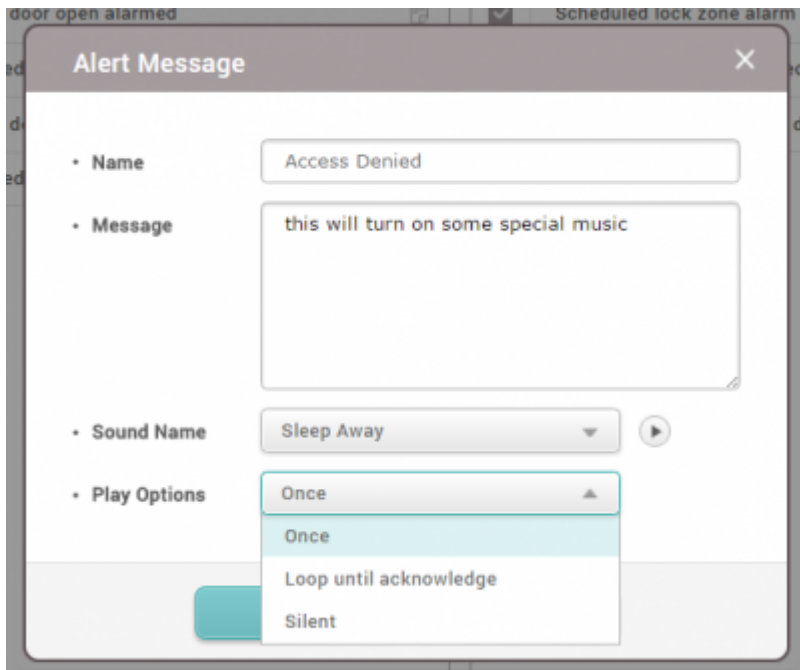

From:  
<https://kb.supremainc.com/knowledge/> -

Permanent link:  
[https://kb.supremainc.com/knowledge/doku.php?id=ko:how\\_to\\_configure\\_alerts](https://kb.supremainc.com/knowledge/doku.php?id=ko:how_to_configure_alerts)

Last update: **2018/07/12 16:49**