


.....	1
.....	1
.....	2
.....	3

, [BioStar 2](#), ,

1. (TIME ATTENDANCE)

2.

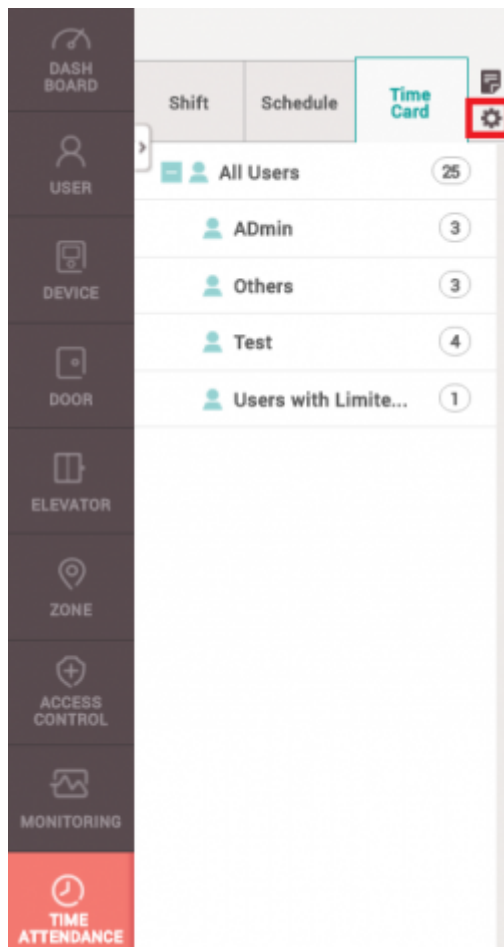

3.

4. + (+ Register)

Setting

Unregistered Devices

No Unregistered Device.

Registered Devices

Unregister

Setting

	Device Name
<input checked="" type="checkbox"/>	BioEntry W2 544108066 (192.168.14.201)
<input checked="" type="checkbox"/>	BioStation 2 546832593 (192.168.14.195)
<input checked="" type="checkbox"/>	BioStation A2 541531061 (192.168.14.222)

(Registered Devices)

가 (Available T&A Mode by device type)

:

가 :

- 가
1. (T&A Mode) (By User)

2. (T&A Required) (Yes)

3. 1 (Code 1) (Label) Checking In

4. 1 (Code 1) (T&A type) (Check In)

5. 2 (Code 2) (Label) Checking Out

6. 2 (Code 2) (T&A type) (Check Out)

7. (Apply)

Setting

T&A Mode

By User

T&A Required

Yes

T&A Event

T&A Event Key	Label	T&A type
Code 1	Checking In	Check In
Code 2	Checking Out	Check Out
Code 3		None
Code 4		None

Apply



Cancel

가 Check In Check Out ,

, , , , , 6가 가 .

(By User): 가 (T&A Required) (Yes) , 가

(By Schedule): (Schedule) > 가(Add Schedule) (Setting) >

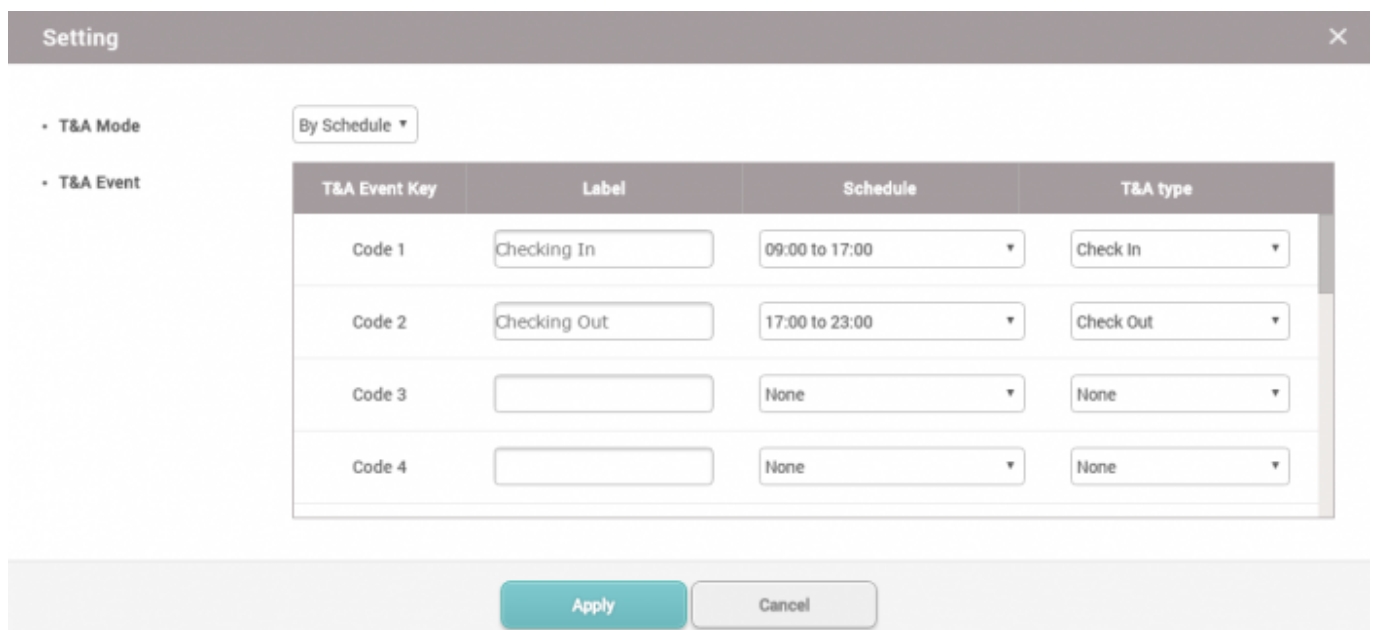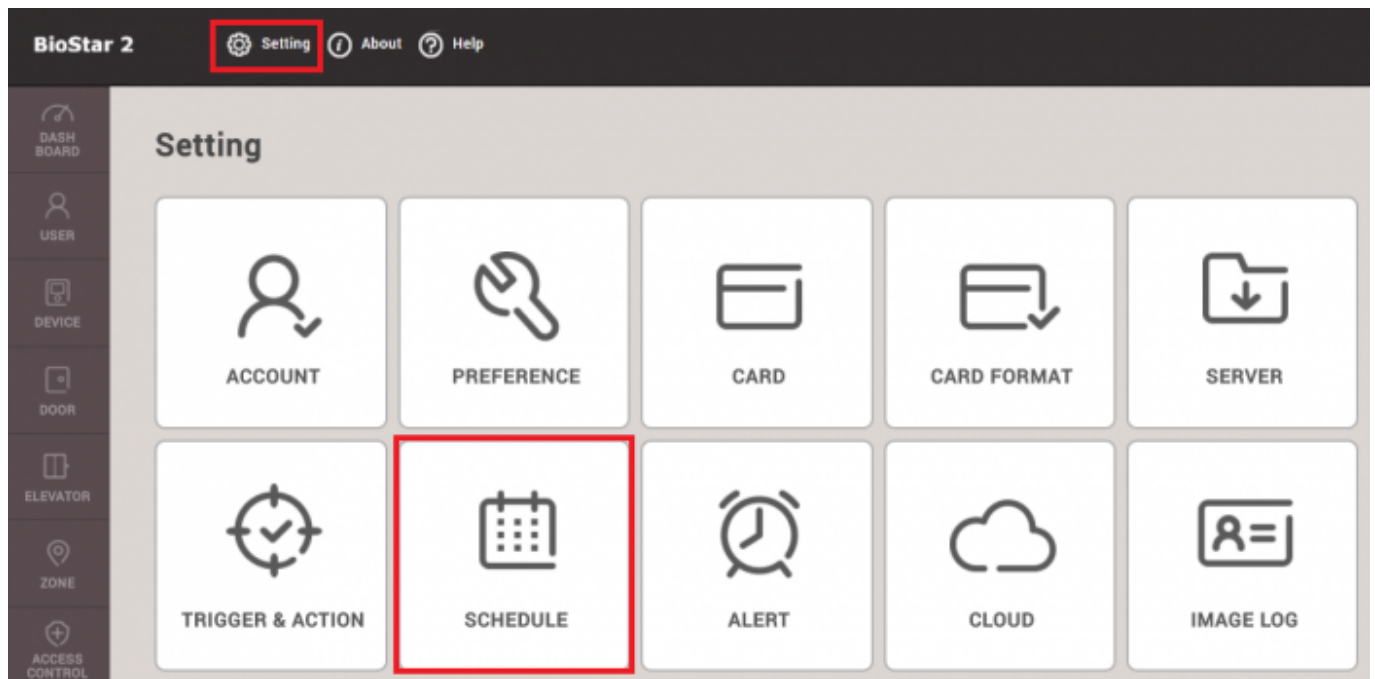

(**Last Choice**): 가 .  
 가 Check In , 가  
 Check In .

(**Fixed**): 가 .

(**Not Use**): .  
 ( ) ( ) .

From:

<http://kb.supremainc.com/knowledge/> -

Permanent link:

[http://kb.supremainc.com/knowledge/doku.php?id=ko:how\\_to\\_configure\\_a\\_t\\_a\\_device](http://kb.supremainc.com/knowledge/doku.php?id=ko:how_to_configure_a_t_a_device)

Last update: **2019/03/14 10:49**